


3 COMP SINK TO WASH UTENSILS

Wash, rinse, and sanitize with using a 3-compartment sink!

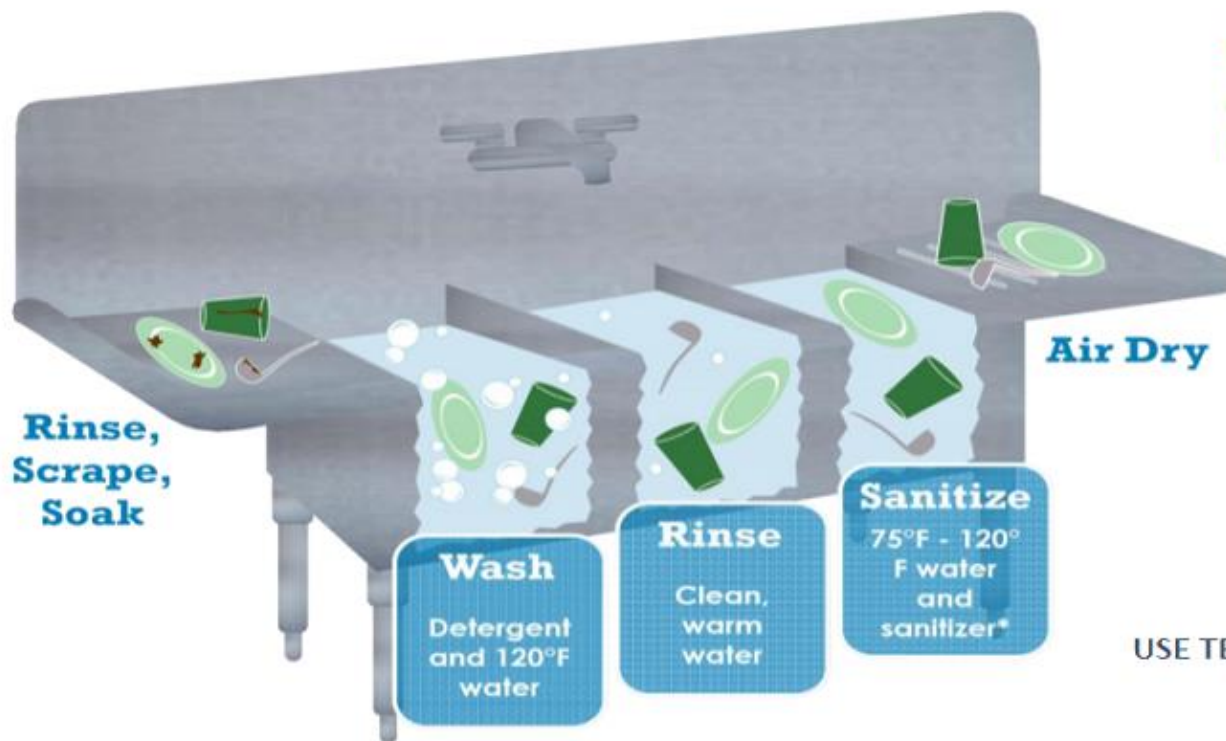

SANITIZE WITH THE RIGHT AMOUNT OF SANITIZER TO PROPERLY KILL GERMS!

CHLORINE/BLEACH: 50-100 ppm

QUATERNARY AMMONIA: 200-400 ppm

IODINE: 25 ppm

**Always follow the sanitizer's label instructions for proper mixing concentrations!*

USE TEST STRIPS TO TEST THE CONCENTRATION



Pickaway County General Health District
Environmental Health Division
110 Island Road, Circleville, OH 43113
740-477-9667 EXT. 225